


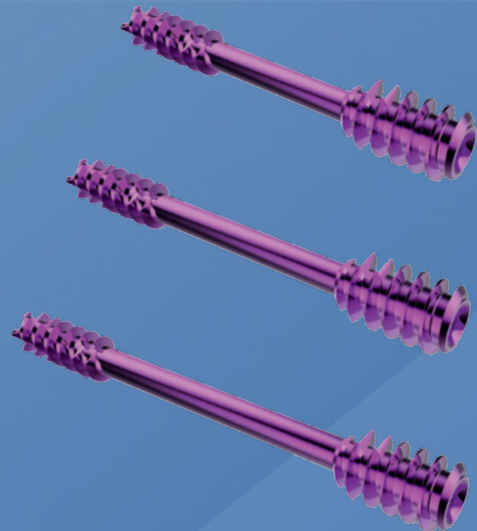

AGOPAQ
STERILIZATION
CONTAINER



**CBS 7.5
SYSTEM**

CBS 7.5 SYSTEM

SAMPLE INDICATIONS:

- SUBTALAR ARTHRODESIS
- ARTHRODESIS OF THE SUBTALAR JOINT
- REVISION OF THE PSEUDO ARTHROSIS
- ARTHRODESIS OF THE CHARCOT ARTHROPATHICS
- CORRECTION OF WRONG POSITIONED ARTHRODESIS
- SURGICAL COMBINATION PROCEDURES WITH OSTEOSYNTHESIS TITANIUM PLATES
- COMPRESSION ARTHRODESIS OF THE TALO-NAVICULAR JOINT AND THE CALCANEO-CUBOIDAL JOINT

AVAILABLE LENGTHS

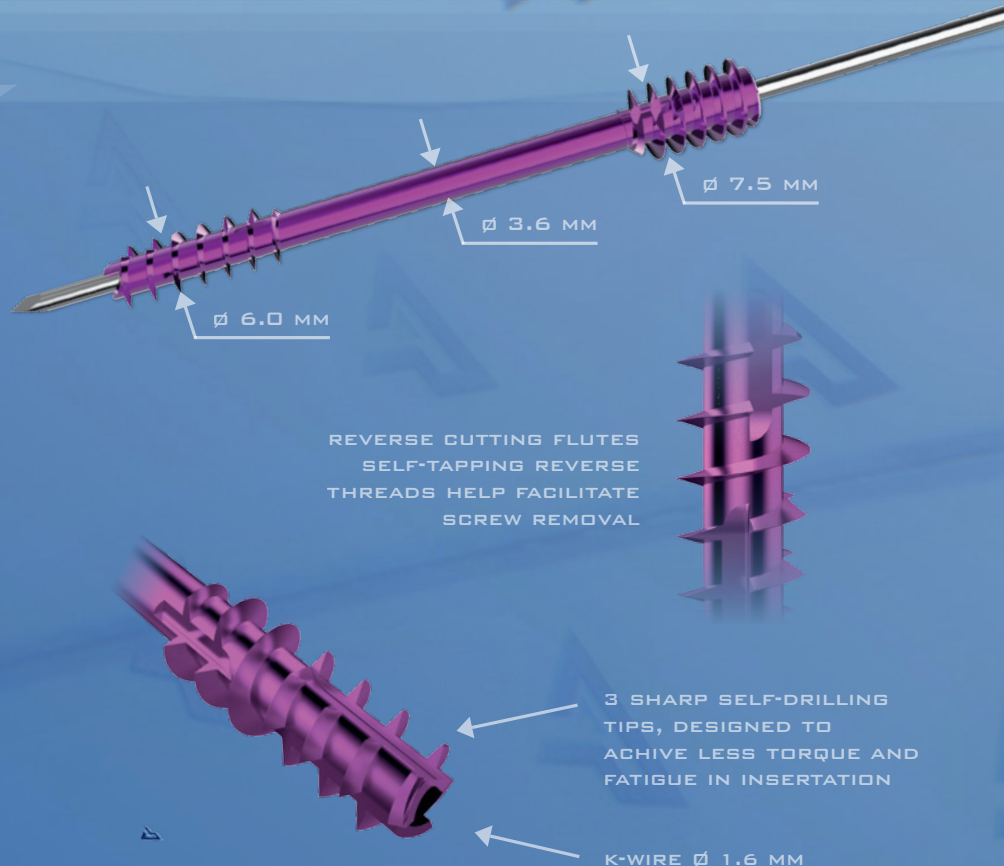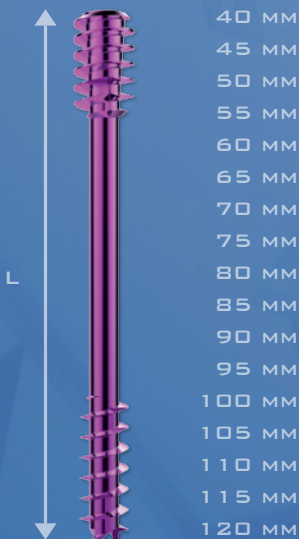

**AGOMED
MEDIZIN-TECHNIK GMBH**

✉ INFO@AGOMED.COM
🌐 WWW.AGOMED.COM
☎ +49 7463 / 267 06 16

ÖSCHWEG 29
78567 FRIDINGEN
TUTTLINGEN / GERMANY